


REVISIONS			
REV.	DESCRIPTION	DATE	APPROVED
A	ADDED ADDITIONAL 6 1/4" THRU HOLES AND 2 TABS	5/23/2013	WS

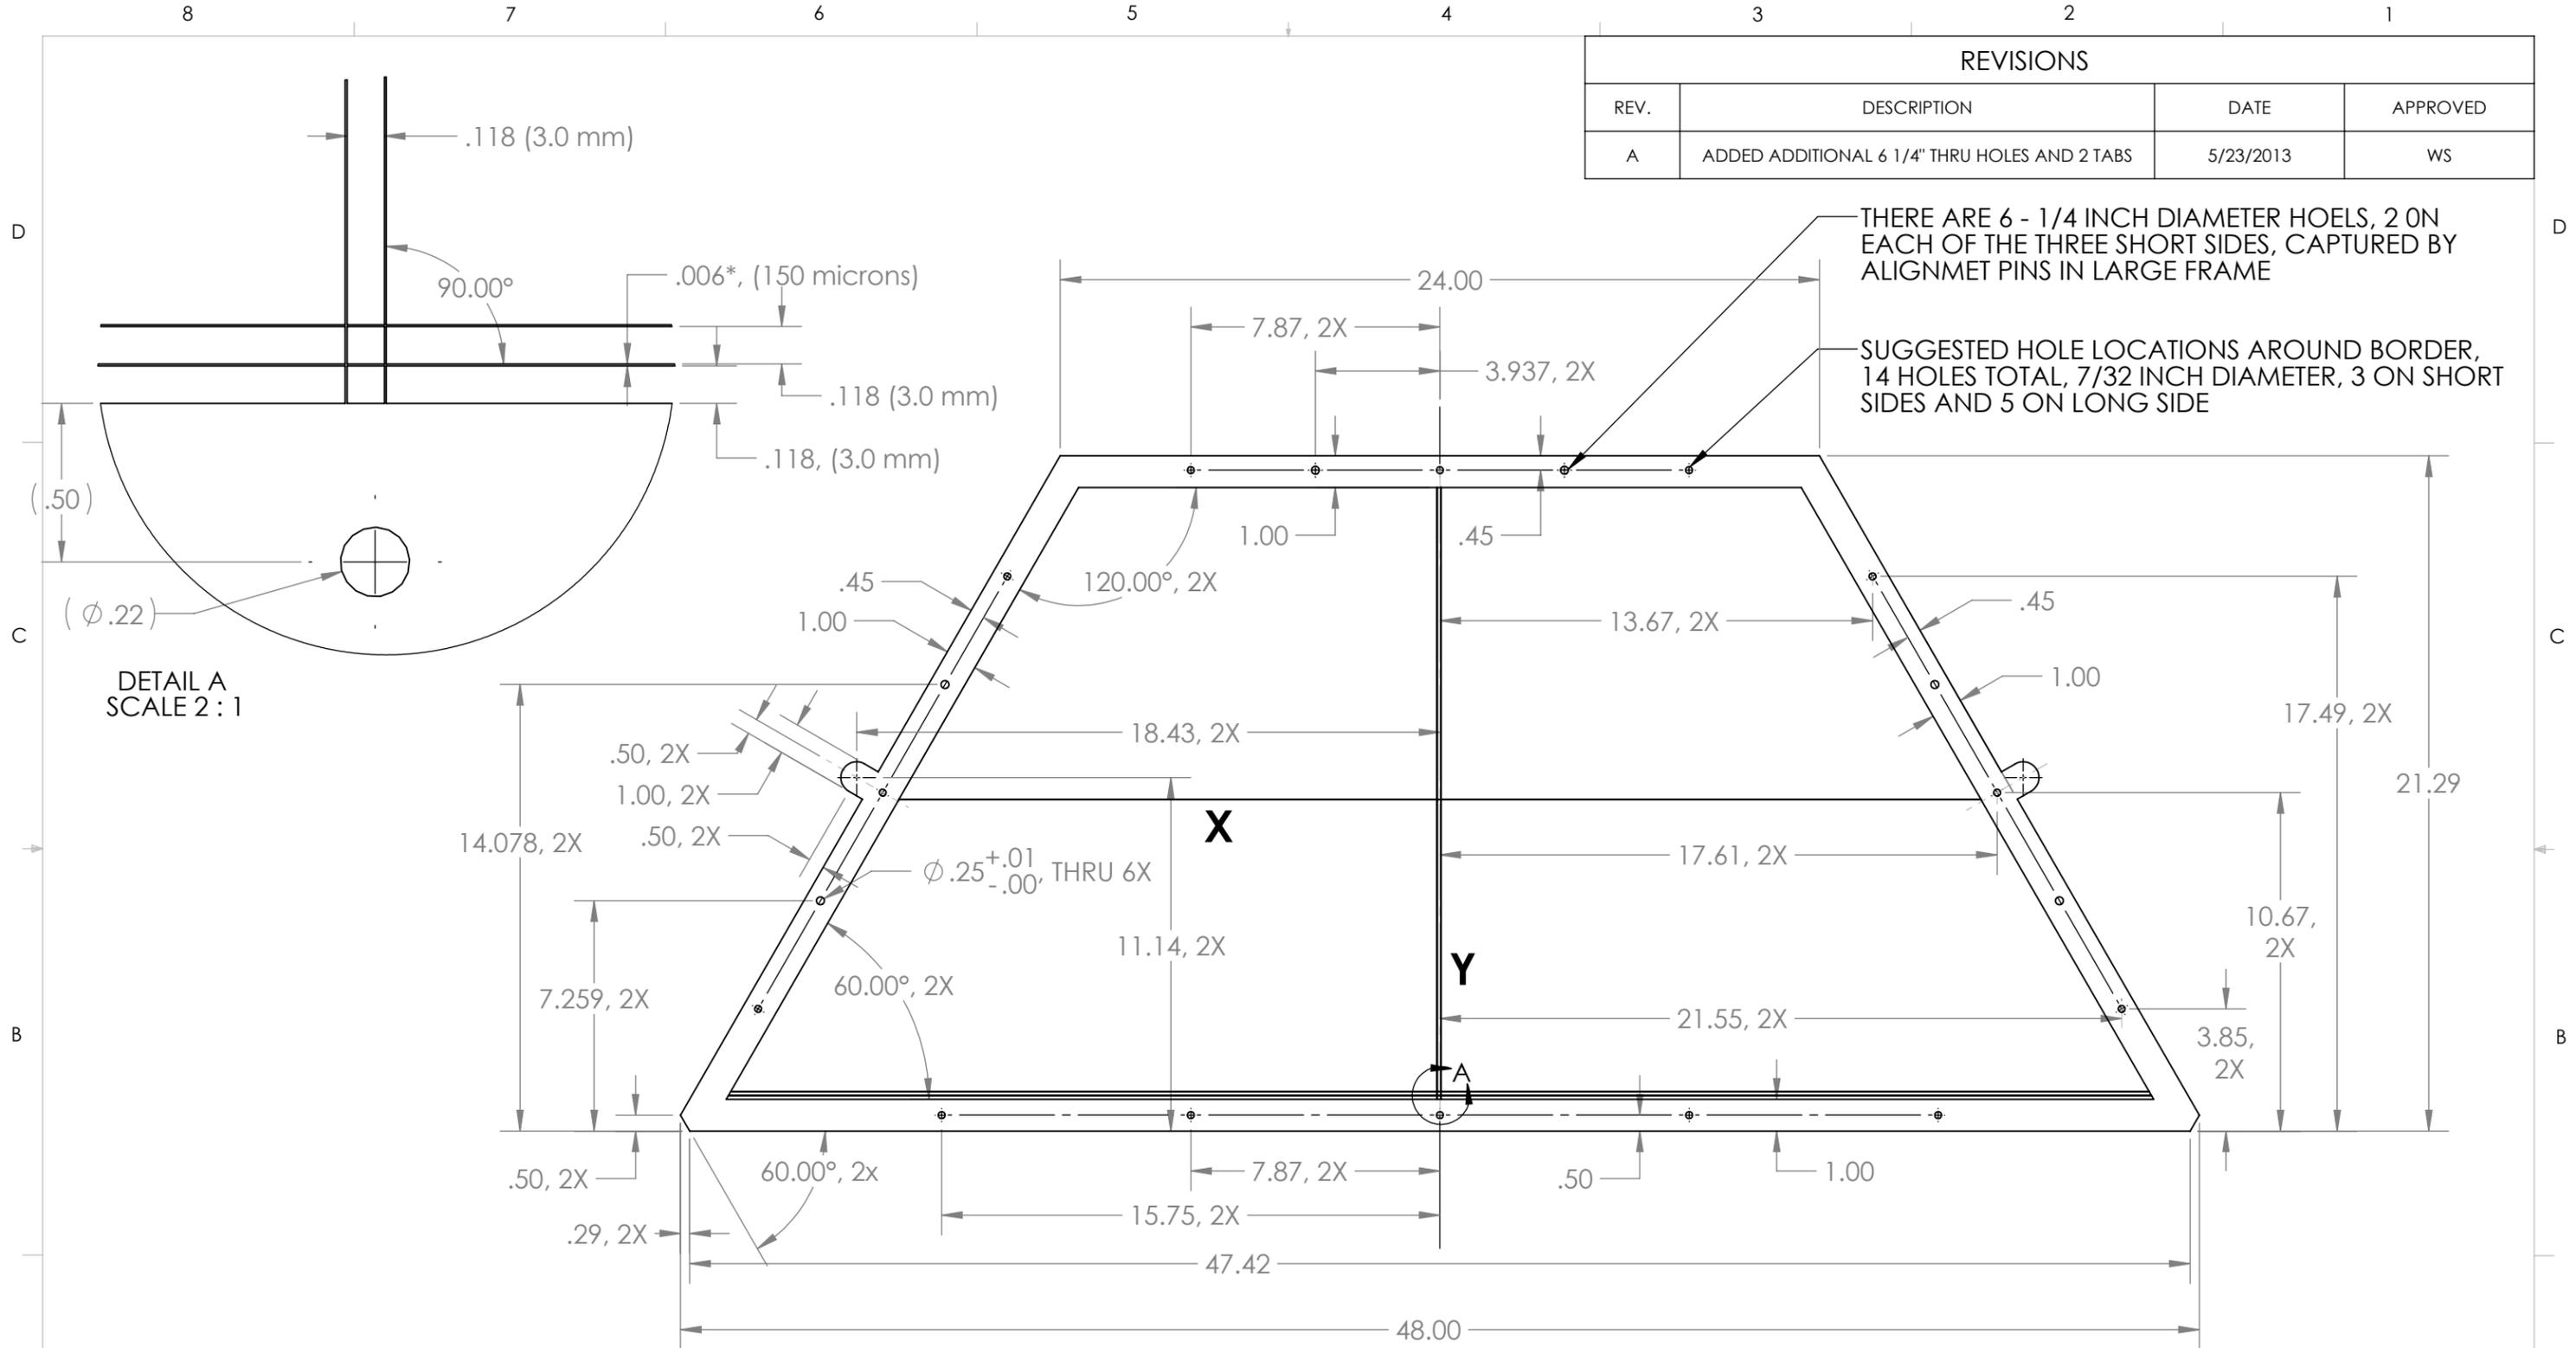

ALL DIMENSIONS IN INCHES

*THICKNESS OF GRID LINES IS DETERMINED BY VENDOR

MATERIAL 304 STAINLESS STEEL FOIL .006in THICK. A CHEMICAL ETCHED X-Y GRID PATTERN IS REQUIRED ON A 3.0 x 3.0 MM SQUARE PATTERN. THE WIDTH OF THE LINES (WIRES) IS 150 MICRONS OR .006 in.

P-25 SUBATOMIC PHYSICS LOS ALAMOS NATIONAL LABORATORY LOS ALAMOS, NM, 87545	DIMENSIONS ARE IN INCHES TOLERANCES UNLESS SPECIFIED: FRACTIONAL ± ANGULAR: MACH ± BEND ± TWO PLACE DECIMAL ± 0.01 THREE PLACE DECIMAL ± 0.003	NAME WALT DATE 4/16/13	half-etched-grid
	MATERIAL 304 STAINLESS STEEL FOIL FINISH QUANTITY REQUIRED 1	DRAWN CHECKED ENG APPR. MFG APPR. Q.A. COMMENTS:	

REV. A
